


VOLUMETRIC PIPETTE (ปีเปตแบบมีกระเปาะ)

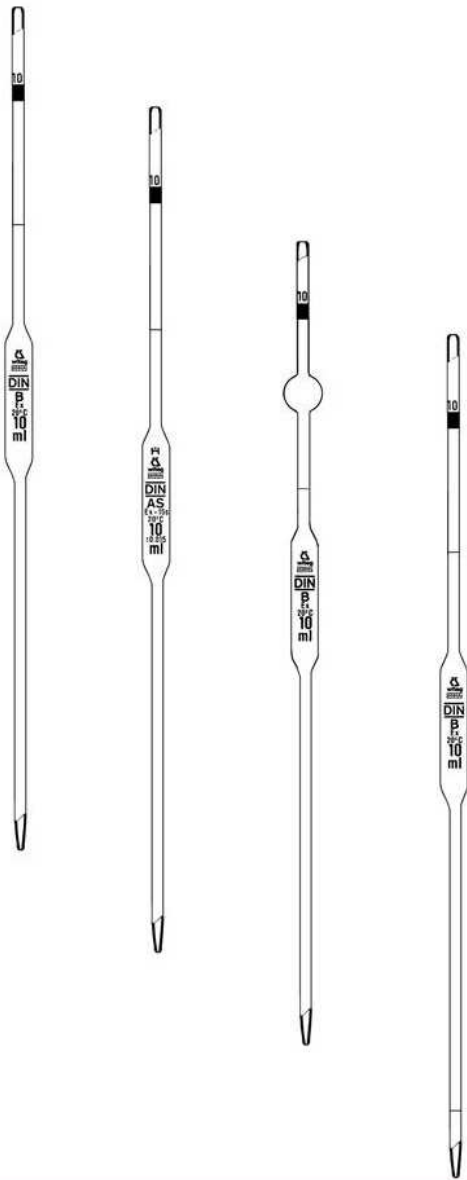

Volumetric pipettes. With ISO-COLOR-Code, acc. to DIN (ISO 648). Calibrated to contain „EX“. With amber stain DIFFICO ring marks and inscriptions, with tempered tips:

1. Class B. DIN 12690. With one mark. Without waiting time
2. Class AS. DIN 12691. Conformity certified. With one mark. Waiting time 15 s. Difficobrown
3. Class AS. DIN 12691. Conformity certified. With one mark. Waiting time 15 s. Difficoblue
4. Class B. With two marks. Without Waiting time
5. Class AS. With two marks. Waiting time 15 s
6. With security bulb

Capacity ml	1.	2.	3.	4.	5.	6.
0.5	3.530.005	3.535.005	3.535.005 BL	3.550.005	3.555.005	* **K
1	3.530.010	3.535.010	3.535.010 BL	3.550.010	3.555.010	* **K
2	3.530.020	3.535.020	3.535.020 BL	3.550.020	3.555.020	* **K
3	3.530.030	3.535.030	3.535.030 BL	3.550.030	3.555.030	* **K
4	—	3.535.040	3.535.040 BL	—	—	—
5	3.530.050	3.535.050	3.535.050 BL	3.550.050	3.555.050	* **K
6	—	3.535.060	3.535.060 BL	—	—	—
7	—	3.535.070	3.535.070 BL	—	—	—
8	—	3.535.080	3.535.080 BL	—	—	—
9	—	3.535.090	3.535.090 BL	—	—	—
10	3.530.100	3.535.100	3.535.100 BL	3.550.100	3.555.100	* **K
15	3.530.150	3.535.150	3.535.150 BL	3.550.150	3.555.150	* **K
20	3.530.200	3.535.200	3.535.200 BL	3.550.200	3.555.200	* **K
25	3.530.250	3.535.250	3.535.250 BL	3.550.250	3.555.250	* **K
30	—	3.535.300	3.535.300 BL	—	—	—
40	—	3.535.400	3.535.400 BL	—	—	—
50	3.530.500	3.535.500	3.535.500 BL	3.550.500	3.555.500	* **K
100	3.530.900	3.535.900	3.535.900 BL	3.550.900	3.555.900	* **K

To order products with individual certificates please add an „IC“ at the end of the respective cat. no., e.g. * **K IC. A batch certificate is included with any standard pack

ISO 9000. It is a must for the documentation of any control of inspection, measuring and test equipment. witeg Labortechnik GmbH prints on all class A/AS volumetric instruments a date-coded batch number for perfect product identification.

Another advantage for your quality laboratory acc. to EN ISO 9000.